


A/V RACK AREA  
RM 2.218A

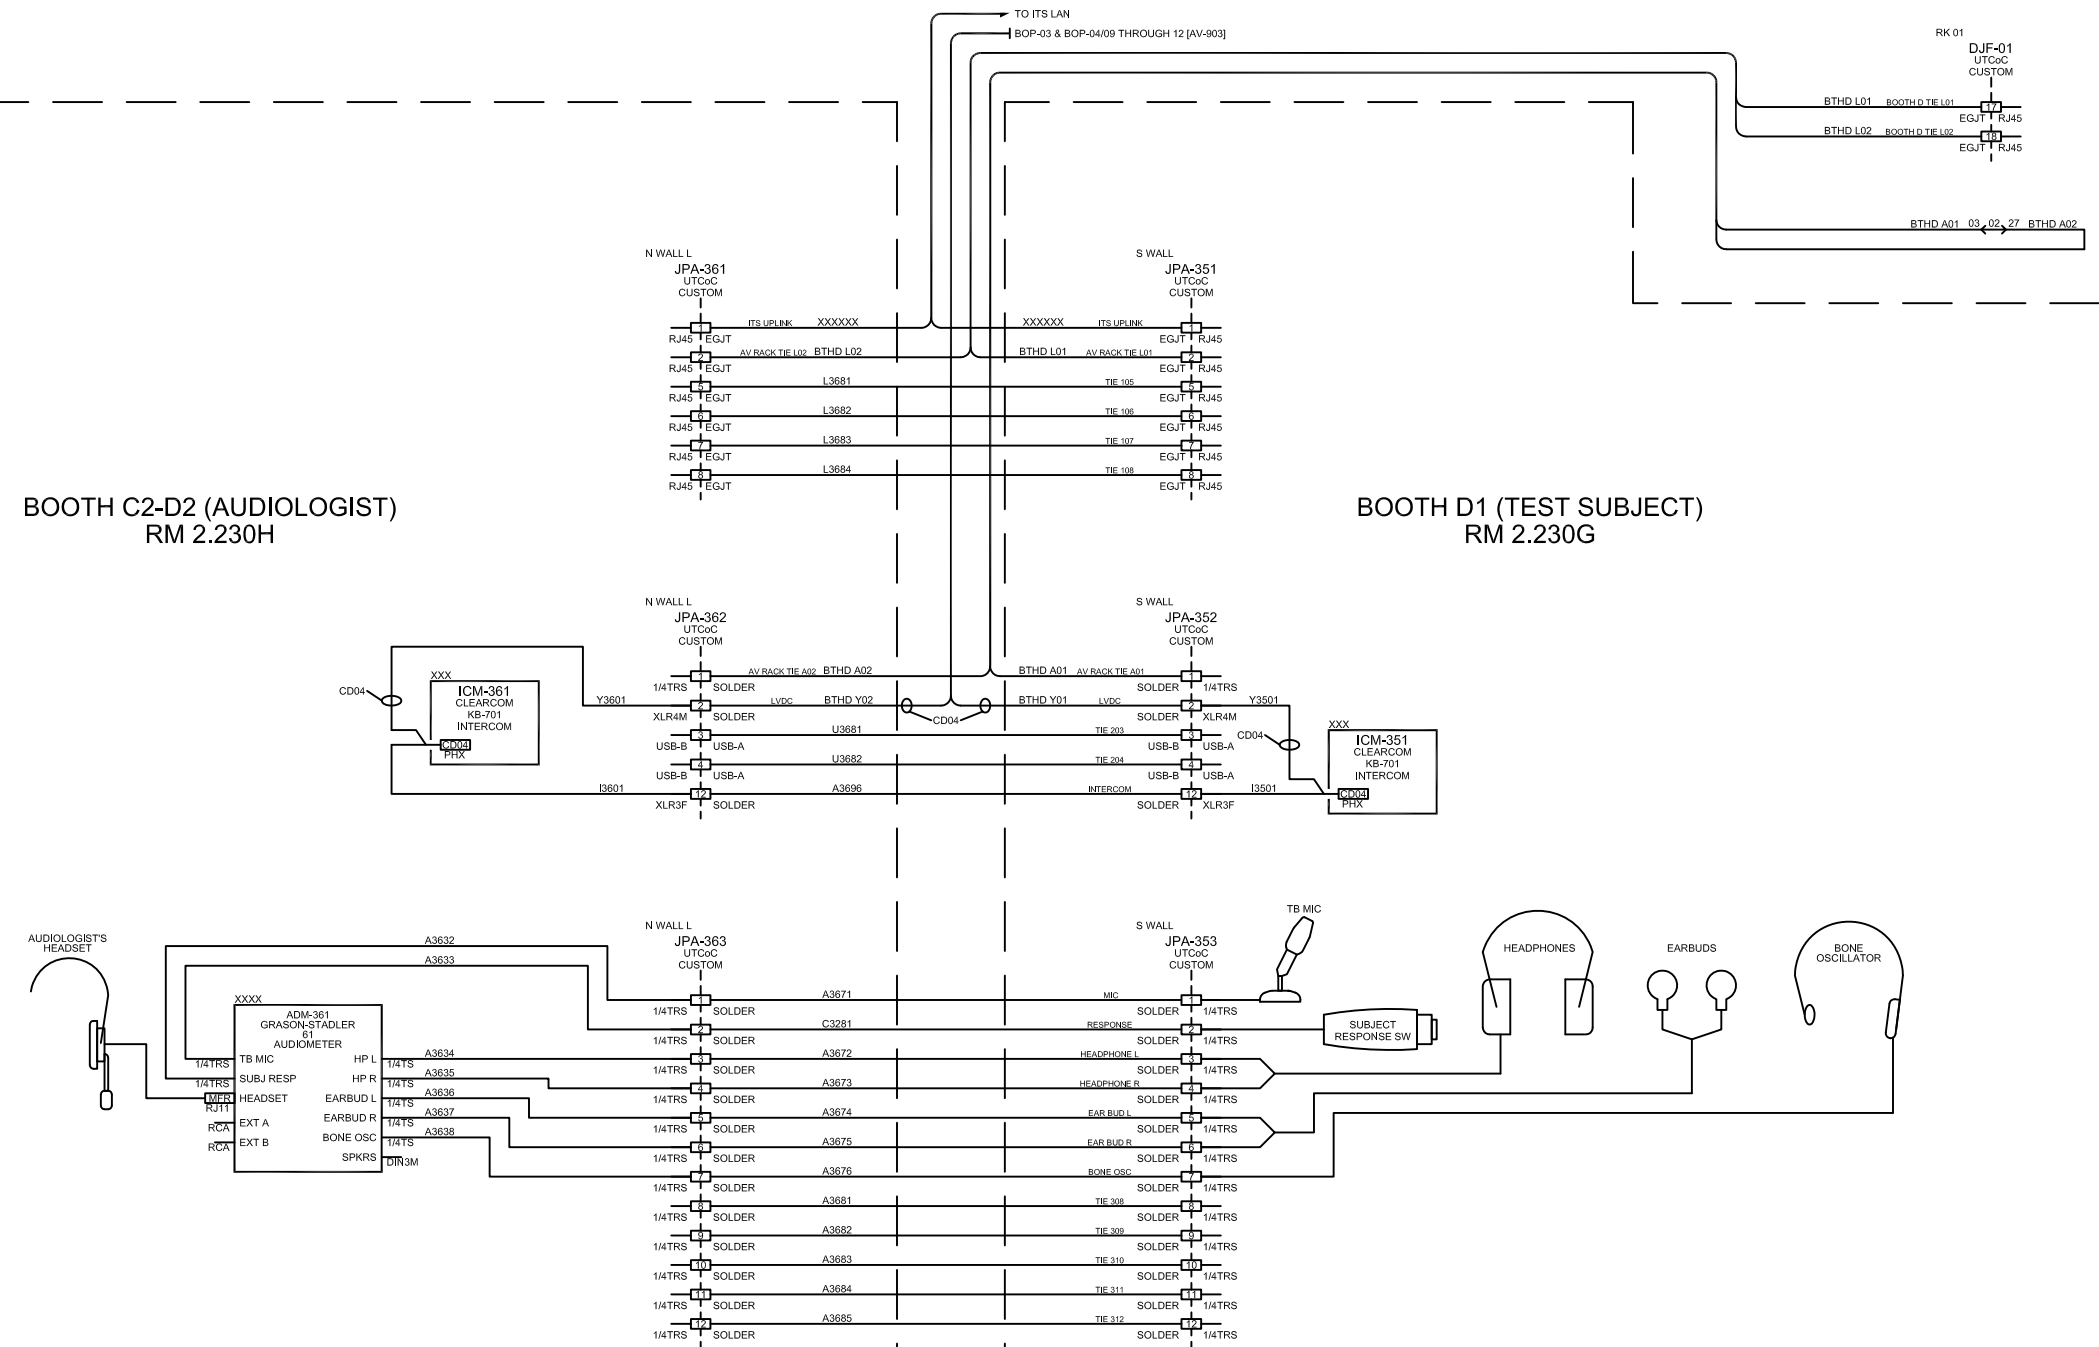

Approved:	H Thompson
Date of Origin:	28 Jan 15
Moody College of Communication CMA2 CSD Clinic	CSD-AV-131D Audiology Suite D
11506 Sierra Nevada Austin, TX 78759 512.401.0713 broadcastfax@austin.rr.com	Last Update: XXXXXX
BROADCAST SOLUTIONS	Engineer:
	XXXXXX